


LGD4033 HPLC Report

Test time: 12/12/2018, 12:21
Product Name :LGD4033
Analyst :LJ
Column: :GSA46250BI017013, C18, 4.6*250mm, 5um
Solvent A :100% Acetonitrile
Solvent B :0.1% Trifluoroacetic in 100% Water
Gradient : A B
0.0min 5% 95%
25.0min 95% 5%
25.1min 100% 0%
30.0min Stop
Flow Rate :1.0ml/min
Wavelength :220nm
Temperature :37°C
Concentration :1mg/ml
Sample Volume :10ul

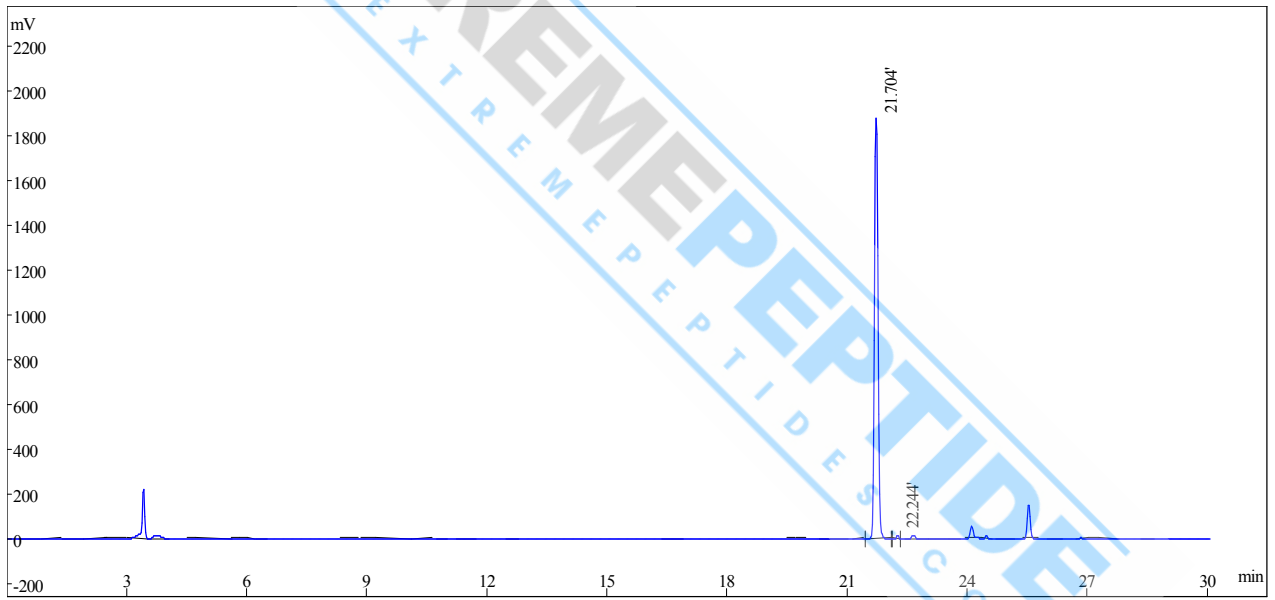

Number	Stay time	Concentration	Peak area	Peak height
1	21.704	99.19	11990142	1883188
2	22.244	0.8078	97643	22233
Total		100	12087785	1905421